



Spotxel® Reader 3.3

Image-Based Microplate Reading and Assay Analysis

User Manual

6 August 2026 - Rev. 1.0

Spotxel® Reader is designed solely for research purposes. It is not intended or approved for the diagnosis of disease in humans or animals.

Copyright 2017-2026 SICASYS Software GmbH. All Rights Reserved.

SICASYS Software GmbH
Geschwister-Scholl-Str. 1
76726 Gernersheim
Germany

Phone +49 (7274) 973 8893
Email info@sicasys.de
Web www.sicasys.de

Contents

Introduction	3
Camera	6
Image Analysis	9
Assay Setup	14
Standard Curve	20
Well Data	22
Assay Report	25
Purchases	28
Settings	31
Appendix A — Third-Party Software Notices	36

Introduction

Product overview, page navigation, and the main changes in Spotxel Reader 3.3.

Spotxel® Reader is a free app for microplate-reader workflows and image-based assay analysis.

The unpaid version is feature-complete and includes a small advertising placement. Paid access removes this advertising placement.

The app is organized into **pages**, also called **screens**. Most pages correspond to steps in the assay workflow. **Purchases**, **Settings**, and **Info** provide supporting functions and information.

To move between pages, touch or click a menu band or the status lane, then drag horizontally.

You can also open the navigation menu and select a page directly. On each page, the navigation menu can be opened in two ways: double-click or double-tap a menu band, or swipe inward from the left edge of the app.

Each page contains one or two menu bands. The buttons in these bands provide the available actions for that page.

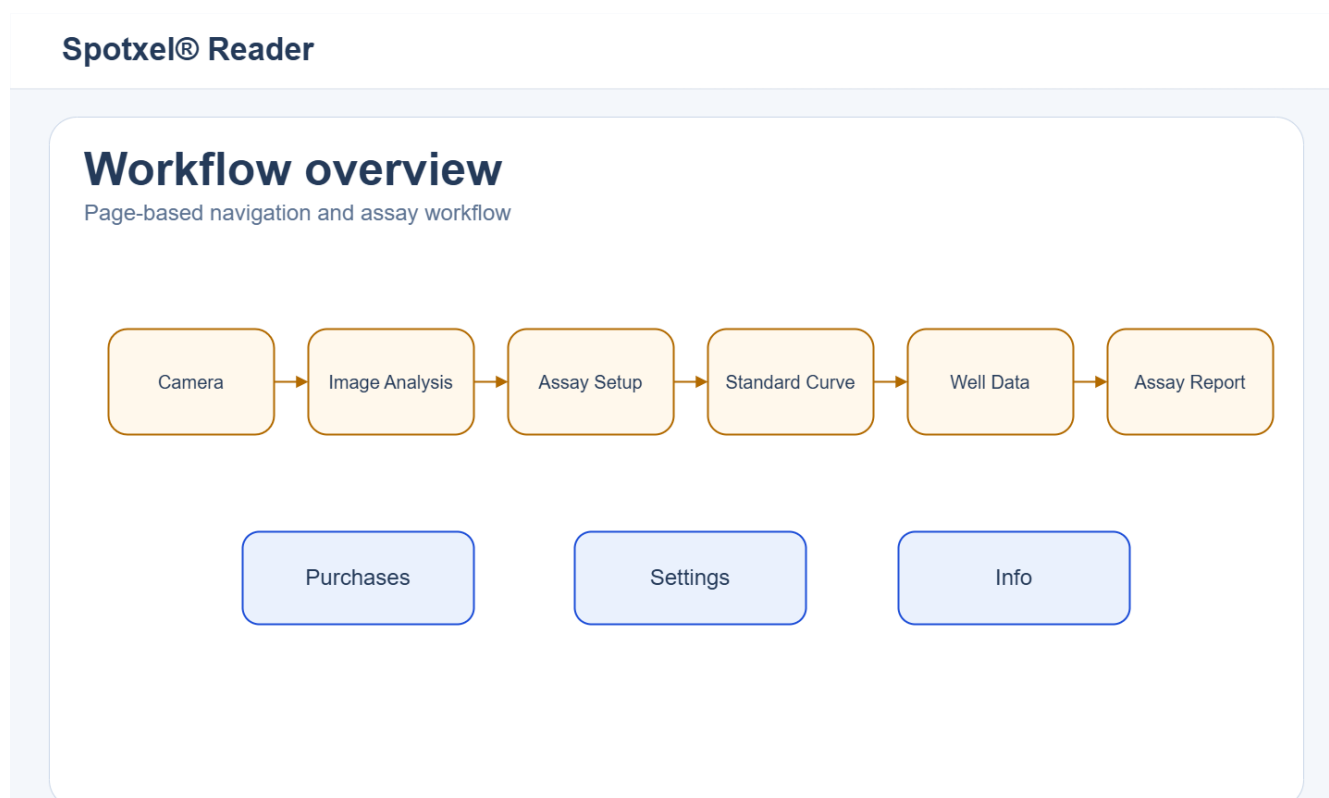


Figure 1. Spotxel Reader page navigation and assay workflow.

Overview of pages

- **Camera:** Preview the plate, prepare image capture with an orientation grid, and capture an image for analysis.

- **Image Analysis:** Select the measured color and quantify well signals from a plate image.
- **Assay Setup:** Create or import an assay design, define standards and unknowns, and calculate unknown concentrations.
- **Standard Curve:** Review the calculated standard curve, inspect unknowns, and select the polynomial degree.
- **Well Data:** Review, sort, import, and export well concentration and signal values.
- **Assay Report:** Choose report sections and export assay data as a PDF report.
- **Purchases:** Review app access, purchase paid access, refresh the product catalog, and restore purchases.
- **Settings:** Configure appearance, layout orientation, workspace, camera device, grid defaults, and troubleshooting.
- **Info:** View version and copyright information, open Help or the navigation menu, share the app, and access product resources. This is the app's starting page.

Actions of Info page

Help

Shows guidance for this page.

Menu

Opens the navigation menu.

Share

Shares Spotxel® Reader or opens the product link.

Links

Use the links on this page to open the privacy policy, product website, third-party license information, and user manual.

New in version 3.3

Spotxel® Reader 3.3 includes several improvements that were not available in versions 1.x or 2.x.

Licenses and access

- Spotxel® Reader is now a free app on all supported platforms.
- The unpaid version is feature-complete and includes a small advertising placement.
- Paid access removes the advertising placement.
- Paid access is available either as a perpetual license or as a 3-month subscription.

User interface

- Multiple color profiles and appearances.
- Workspace setting for organizing images, grid profiles, assay designs, reports, and exports.
- Portrait mode support on desktop versions.
- Switching between portrait and landscape mode.

For desktop use, landscape mode is still recommended because it makes better use of the available screen space.

These options can be configured on the **Settings** page, together with:

- Camera device selection.
- Grid type selection for microplates.

New Image Analysis tools

- **Image Tools:** Rotate and flip the image.
- **Grid Tools:** Rotate and flip the grid.
- **Align Grid:** Automatically align the grid to the plate image. This feature is currently available as a beta version.

Camera

Preview the plate, align the orientation grid, and capture an image.

For reliable image analysis, the plate should be captured as straight and evenly framed as possible. The **orientation grid** helps you check the plate position before capture. It is a 12 × 8 guide grid with highlighted wells at the corners and center.

The initial grid may not align perfectly with the plate because of camera parameters, lens distortion, and capture distance. Use the grid tools to adjust the grid size, position, and distortion before capturing the image.

Workflow

Start the camera preview, align the orientation grid with the plate, capture an image, review the capture, then accept it for image analysis.

Captured images



Windows and macOS

On desktop systems, accepted image captures are stored in the workspace image folder configured on the **Settings** page.



Android

On Android, accepted image captures are stored under **Pictures/Spotxel Reader**.



iPhone and iPad

On iOS, accepted image captures are saved under **On My iPhone/Spotxel Reader/Images** or **On My iPad/Spotxel Reader/Images**, depending on the device.

To analyze an accepted capture later, open the **Image Analysis** page and select **Open Image**.

Camera permission

The app needs permission from the operating system to use the camera.

On macOS, if camera permission has not been granted, a system dialog appears when **Start** is selected.

On Windows, a system dialog may appear the first time the app is started.

On all platforms, camera permission must be granted before the camera can be used. If permission was denied, enable camera access in the operating system privacy or camera settings, then start the camera preview again.

Actions for Camera

▶ Start

Starts the live camera preview. If camera permission is required, the operating system may ask for permission before the preview can start.

○ Capture

Captures the current preview image for review.

i Capture Info

Shows camera and last-capture details.

✓ Accept

Sends the reviewed capture to Image Analysis.

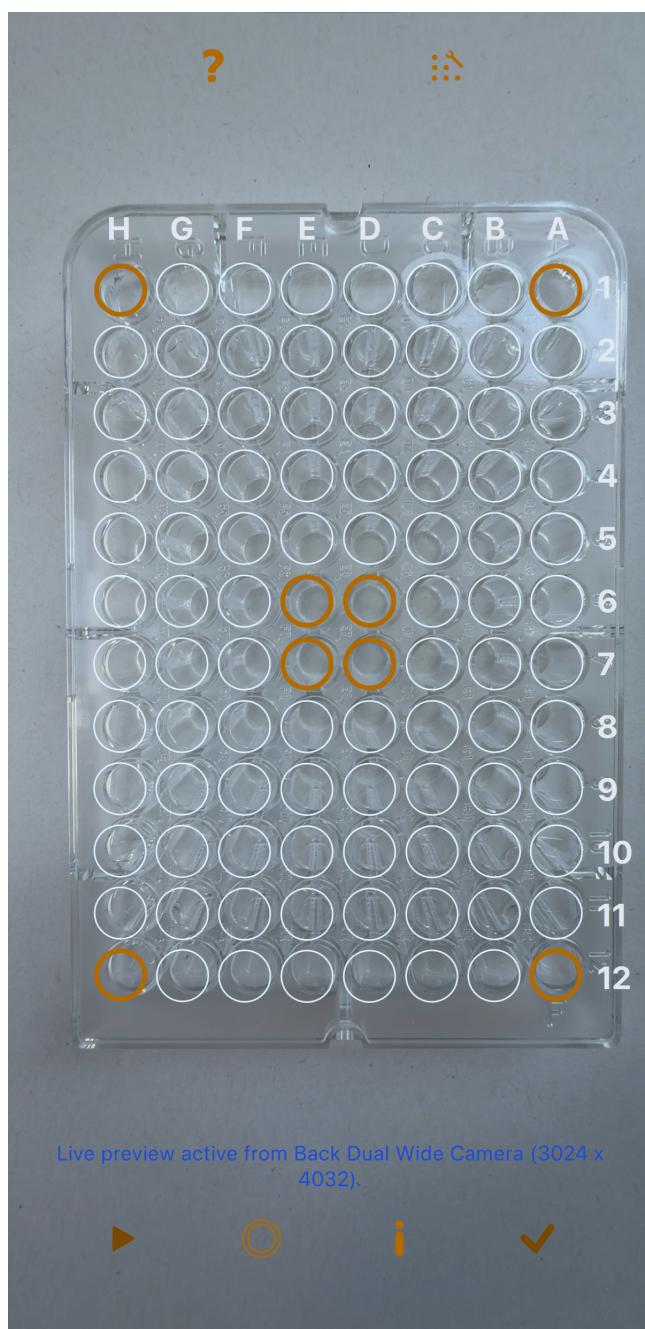


Figure 2. The Camera page with the orientation grid positioned over an empty microplate.

Page and grid actions

Help

Shows guidance for this page.

Grid Tools

Opens the manual grid controls.

Grid Tools

Resize Grid

Changes the grid size with the mouse wheel or pinch gesture.

Move Grid

Moves the grid by dragging on the preview.

Distortion

Adjusts the grid distortion to better match the plate image.

Reset Grid

Restores the default grid for the preview.

Camera device

The default camera is used on this page.

To use another camera, open the **Settings** page and select the device in the **Camera Device** section. Depending on the platform and device, this can be a built-in camera, a USB-connected camera, or a network-connected camera.

Image Analysis

Load an image, align the well grid, select the measured color, and quantify signals.

Workflow

Open an image, align the well grid to the plate, select the measured color, then run the analysis.



Windows and macOS

On desktop systems, **Open Image** opens a file dialog for selecting a source image.



Android

On Android, **Open Image** opens the Android system file picker and shows supported image files.



iPhone and iPad

On iOS, **Open Image** offers **Choose from Photos** and **Choose from Files**. The Files picker starts under **On My iPhone/Spotxel Reader/Images** or **On My iPad/Spotxel Reader/Images**, depending on the device. Accepted camera captures are stored there, and you can also browse iCloud Drive and other Files providers.

Grid alignment settings can be saved to a JSON file and reused later. See **Grid profiles** below.

After analysis, inspect the calculated well signals by zooming and panning the image. Detected well boundaries are highlighted with the main color of the selected color profile.

Sample data

A sample microplate image can be [downloaded here](#).

A package of sample images for testing Align Grid is available for [download here](#).

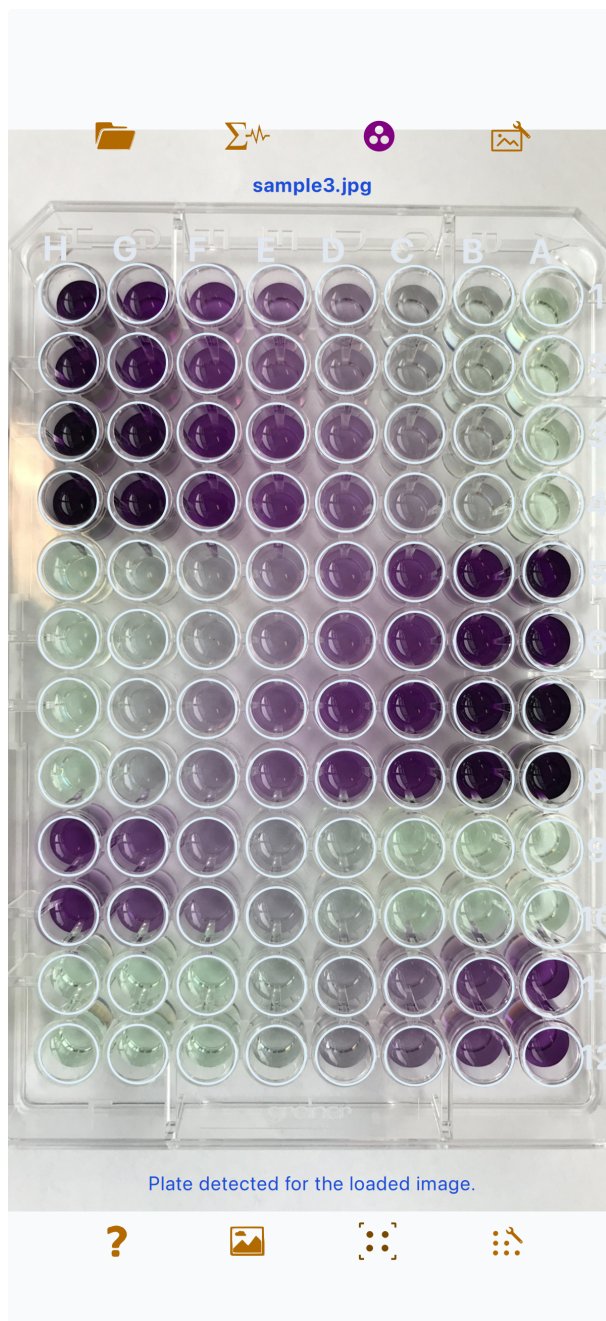


Figure 3. The Image Analysis page after loading a plate image and aligning the well grid.

Image actions

 **Open Image**
Loads a source image.

 **Analyze**
Calculates well signal values when the image, grid, and measured color are ready.

 **Measured Color**
Selects the color channel used for quantification.

 **Image Tools**
Opens image information, pan and zoom, image orientation, and clear actions.

Page and grid actions

The initial grid may not align perfectly with the plate because of camera parameters, lens distortion, capture distance, or image orientation. Use automatic alignment or the manual grid tools to match the grid to the plate image.

Help

Shows guidance for this page.

Align Grid

Automatically fits the grid to the plate image. This feature is currently available as a beta version. **Grid Mode** must be active to use this action. See **Interaction modes** below.

Precondition: The image should show one complete microplate. The full plate outline must be visible and must not be cut off. Avoid images with multiple plates, hands, strong background objects, or other objects that may be mistaken for the plate.

Grid Tools

Opens manual grid editing, grid profile, visibility, reset, and lock actions.

Interaction modes

Image Analysis has separate image and grid interaction modes. These modes help you inspect the image without accidentally editing the grid, and edit the grid without changing the image view.

Image Mode

Pans and zooms the image without editing the grid.

Grid Mode

Moves, resizes, rotates, or distorts the grid.

Grid Locked

Keeps the grid visible but prevents accidental grid edits.

After loading an image and after running analysis, **Image Mode** is activated so you can inspect the image by panning and zooming.

To switch from **Image Mode** to **Grid Mode**, click or tap the grid. To leave **Grid Mode**, click or tap the image outside the grid.

Use **Grid Mode** while aligning the grid. Once the grid is aligned, **Grid Locked** is recommended to freeze the grid and prevent accidental edits.

Image Tools

Image Tools provide image inspection, view control, orientation correction, and clearing actions.

- **Image Info:** Shows information about the loaded image.
- **Show Image Filename:** Shows or hides the loaded image filename near the Image Tools action band.
- **Pan/Zoom mode:** Enables image panning and zooming.
- **Reset View:** Restores the default image view.
- **Rotate 90° CW:** Rotates the image 90 degrees clockwise.
- **Rotate 90° CCW:** Rotates the image 90 degrees counterclockwise.
- **Rotate 180°:** Rotates the image by 180 degrees.

- **Flip Horizontal:** Mirrors the image horizontally.
- **Flip Vertical:** Mirrors the image vertically.
- **Reset Orientation:** Restores the original image orientation.
- **Clear:** Removes the loaded image and clears the current analysis input.

To zoom the image, use the mouse wheel. On a touchpad or touchscreen, use a pinch gesture by moving two fingers apart or toward each other. On a touchpad, you can also slide two fingers upward or downward. Drag the image to pan when pan and zoom are active.

The image view can also be reset by double-clicking or double-tapping the image outside the grid.

Grid Tools

Grid Tools provide manual grid alignment, profile import and export, visibility control, reset, and locking actions.

Grid profiles

- **Save Grid Profile:** Saves the current grid size, position, distortion, and orientation to a JSON file.
- **Load Grid Profile:** Loads a saved grid profile and applies it to the current grid.

The suggested filename for a saved grid profile is based on the original source image name.

On Android, **Save Grid Profile** opens the system file picker with a suggested filename and folder under **Download/Spotxel Reader/Grid Profiles**.

On iOS, **Save Grid Profile** opens **Save As** with a suggested filename and folder, such as **On My iPhone/Spotxel Reader/Grid Profiles** or **On My iPad/Spotxel Reader/Grid Profiles**.

A grid profile stores the grid configuration only. It does not save the image itself, the image orientation, or any image rotation applied in Image Tools.

Manual grid adjustment

To change the grid manually, select the corresponding tool and use the mouse wheel or a touchpad gesture.

- **Resize Grid:** Changes the grid size. On a touchpad, use two fingers and slide upward or downward. You can also use the more natural pinch gesture by moving two fingers apart or toward each other.
- **Rotate Grid:** Rotates the grid around its center. On a touchpad, use two fingers and slide upward or downward.
- **Distortion:** Adjusts the grid distortion to better match the plate image. On a touchpad, use the corresponding two-finger scroll gesture.

For manual alignment, first align the center wells, such as D6, D7, E6, and E7. Then tune the grid size, rotation, and distortion until the grid fits the whole plate.

Auto-aligned grids

After using **Align Grid**, use these actions if the automatically aligned grid has the wrong orientation:

- **Rotate Grid 180°:** Rotates the grid by 180 degrees.
- **Flip Grid Horizontal:** Mirrors the grid horizontally.
- **Flip Grid Vertical:** Mirrors the grid vertically.

Visibility, reset, and lock

- **Hide Grid:** Hides the grid for better inspection of the image signal. The grid is shown again automatically when **Grid Tools** is opened.
- **Reset Grid:** Restores the grid to the last state used for **Analyze** or **Align Grid**. The grid can also be reset by double-clicking or double-tapping the grid.
- **Lock Grid:** Activates **Grid Locked** to prevent accidental grid edits.

Assay Setup

Annotate wells, define standards, and assign standard concentrations.

Use this page to assign well names, notes, standards, and concentrations for the assay.

During assay setup, you can annotate wells, review detected signal values, and assign concentrations to standard wells. The assay setup can be saved to a CSV file and reused in another analysis.

Sample data

For the [sample microplate image](#), you can download assay setup CSV files for testing:

- [CSV with decimal-point numbers](#)
- [CSV with decimal-comma numbers](#)

Spotxel® Reader can import both decimal-point and decimal-comma floating-point numbers. Values are displayed according to your system locale.

Workflow

A representative assay grid is shown on this page. It reflects the plate layout and lets you edit the assay design independently of the original plate image.

You can resize the grid with the mouse wheel or a pinch gesture.

To move the grid, drag it as follows:

- On mobile devices, tap a point within the grid and drag.
- On desktop systems, click a row or column label, or click a point within the grid but outside a well boundary ring, then drag.

To set up an assay from scratch, first define the maximum standard concentration and concentration unit. Then annotate the wells and assign concentrations to the standards.

A typical setup workflow is:

1. Set the maximum standard concentration and concentration unit.
2. Use **Annotation** mode to name the assay and annotate wells.
3. Use **Concentration** mode to assign concentrations to standard wells.
4. Use **Signal** mode to review detected signal values, if image analysis data is available.
5. Run **Analyze** to calculate the standard curve and derive unknown concentrations.
6. Export the setup if you want to reuse it later.

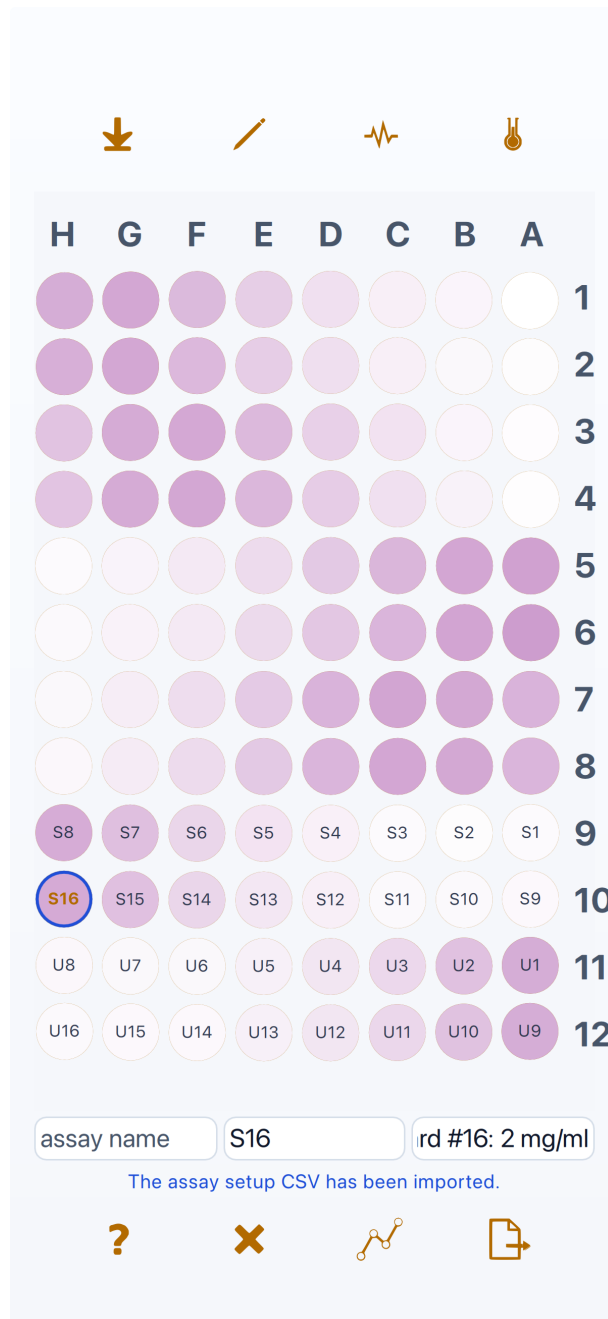


Figure 4. The Assay Setup page in Annotation mode.

Well colors

The selected well is highlighted with the main color of the current color profile.

Standard wells are highlighted with the message color of the current color profile, similar to the text color used in the status lane.

Setup modes and import

↓ Import Setup

Loads assay setup data from a CSV file.

/ Annotation

Edits the assay name, well names, and well notes.

Signal

Reviews detected signal values when image analysis data is available.

Concentration

Assigns concentrations to standard wells.

Page actions

Help

Shows guidance for this page.

Clear

Clears editable assay setup entries while keeping detected signal values.

Analyze

Calculates the standard curve from the current setup and derives unknown concentrations.

Export Setup

Saves the assay setup as a CSV file.

Assay design

An assay design is the reusable assay setup data: named wells, optional notes, standards, and standard concentrations. It can be exported to a CSV file and reused later.

Measured signal values and calculated concentrations are not included in an assay design. Export those results from the **Well Data** page.



Windows and macOS

On desktop systems, assay design import and export use the workspace folders configured on the **Settings** page.



Android

On Android, **Export Setup** opens the system file picker with a suggested filename and folder under **Download/Spotxel Reader/Assay Designs**.



iPhone and iPad

On iOS, **Export Setup** opens **Save As** with a suggested filename and folder, such as **On My iPhone/Spotxel Reader/Assay Designs** or **On My iPad/Spotxel Reader/Assay Designs**.

Named wells that do not have a standard concentration are treated as unknowns. Unknown concentrations are calculated only for named unknown wells.

Annotation mode

Use **Annotation** mode to define the assay name and annotate individual wells.

In the **Assay** box, enter the assay name. This name is used when exporting assay data, for example to a CSV file or PDF report.

To annotate a well, click or tap the well to select it. Then enter the well name and optional notes in the input boxes at the bottom.

Example well names are **S1**, **S2**, and **S3** for standards, or **U1**, **U2**, and **U3** for unknowns.

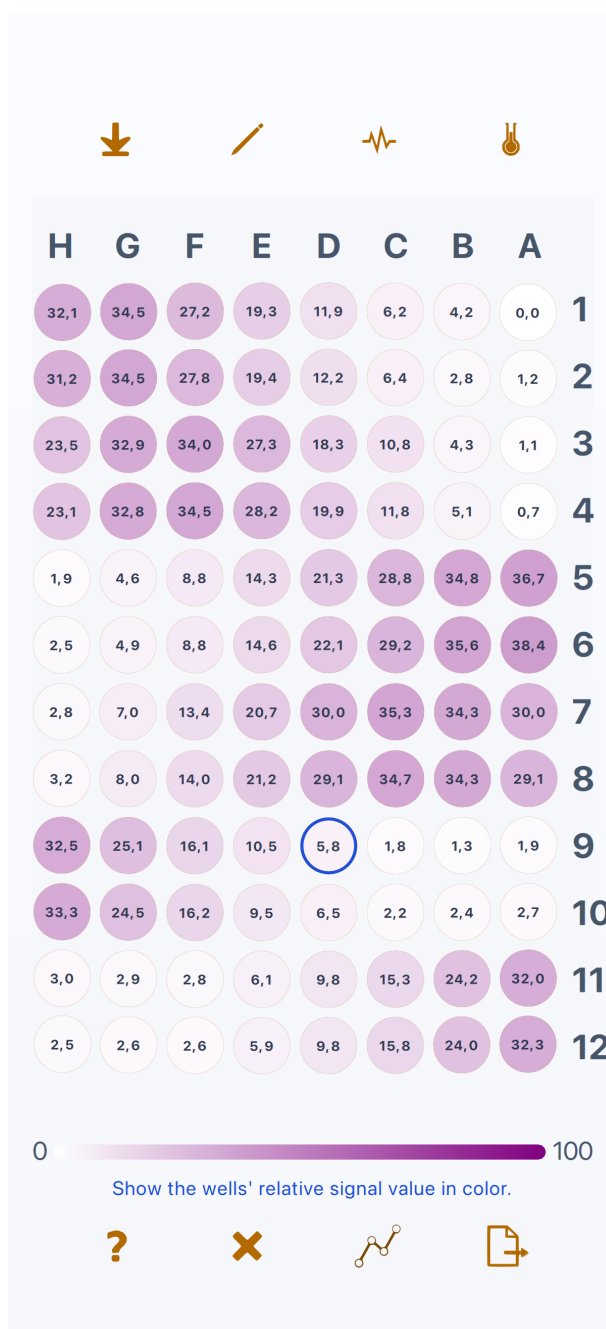


Figure 5. The Assay Setup page in Signal mode.

Signal mode

Use **Signal** mode to review detected well signal values after image analysis.

If image analysis data is available, wells are colored according to their detected signal values and the numeric signal value is shown inside each well.

This mode is useful for checking whether the image analysis result is plausible before calculating the standard curve.

Concentration mode

Use **Concentration** mode to assign concentrations to standard wells.

First, set the maximum standard concentration. Click or tap the maximum concentration value box on the concentration slider to open the value setting dialog. Enter the maximum value, then choose **OK**.

By default, the maximum concentration is **10 ug/mL**. Select the concentration unit in the adjacent list box if needed.

To define a standard, click or tap a well to select it, then use the concentration slider or enter the value directly in the **well concentration** box at the bottom.

The concentration value must be between zero and the configured maximum concentration. The selected concentration is shown under the well name.

Standard wells are highlighted with the message color of the current color profile. To remove a standard concentration, select the well and delete its concentration value.

Calculating unknown concentrations

After defining the assay design, run **Analyze** to calculate the standard curve from the standards and derive concentrations for the unknowns.

The standards, unknowns, and standard curve are shown on the **Standard Curve** page. There you can inspect signal and concentration values, select a different polynomial degree for the standard curve, and recalculate unknown concentrations.

Only named unknown wells are included in the concentration calculation. To calculate a concentration for an unknown well, assign it a name such as **U1** or **U2**.

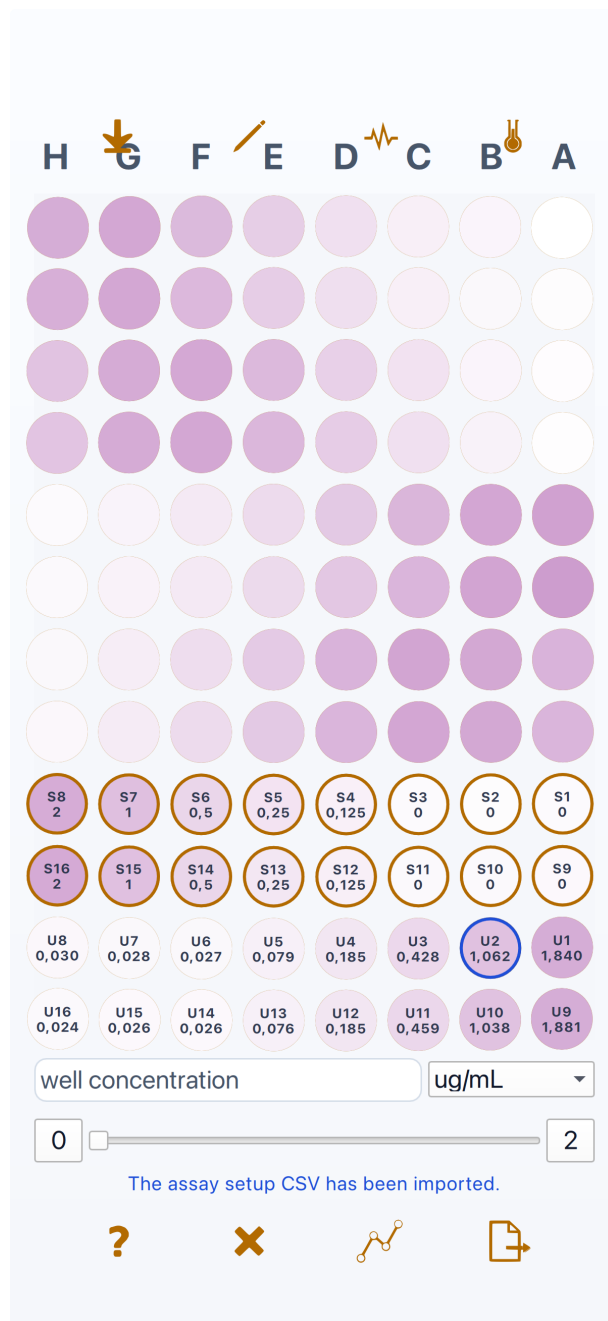


Figure 6. The Assay Setup page in Concentration mode.

Standard Curve

Inspect the fitted curve and recalculate unknown concentrations.

Workflow

This page is updated automatically when valid assay setup and signal data are available.

Review the standard curve, inspect the standard and unknown markers, and adjust the polynomial degree if needed. Then continue to the **Well Data** or **Assay Report** pages.

Actions

Help

Shows guidance for this page.

Show Unknowns / Hide Unknowns

Shows or hides derived unknown sample markers in the chart.

Reset Zoom

Restores the default chart view.



Polynomial Degree

Selects the regression polynomial degree and recalculates the standard curve.

Standard Curve chart

The chart shows the relationship between measured signal and concentration.

Standards are plotted as markers using their measured signal and assigned concentration. The fitted standard curve is shown as a line through the chart. Unknown samples can also be shown as derived markers.

The horizontal axis shows the measured **Signal**. The vertical axis shows the calculated or assigned **Concentration**.

The standard curve equation is shown at the top of the chart. In the equation, **X** represents the signal and **Y** represents the concentration. **R²** is the coefficient of determination and indicates how closely the fitted curve matches the standard points.

You can zoom the chart with the mouse wheel or a pinch gesture. To restore the default view, double-click or double-tap the chart, or use **Reset Zoom**.

By default, unknown sample markers are hidden. Use **Show Unknowns** or **Hide Unknowns** to control their visibility.

To view the signal and concentration of a marker, hover over it on desktop or tap it on a touch device.

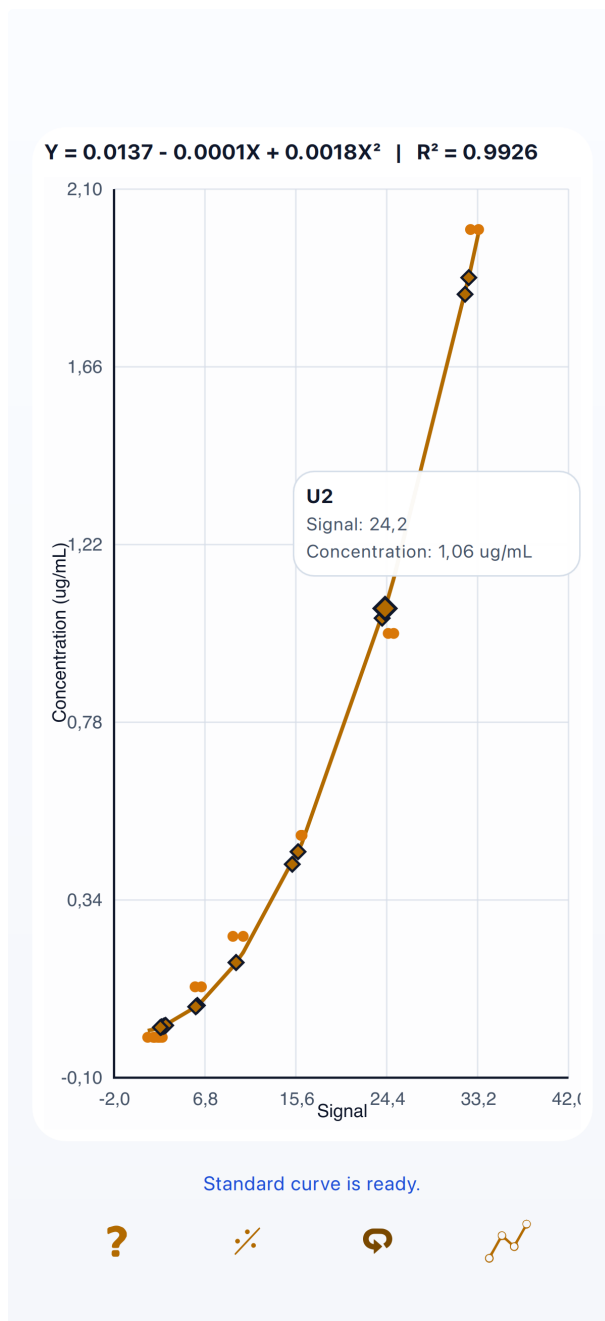


Figure 7. The Standard Curve page with standards, optional unknown markers, the fitted curve, equation, and R^2 value.

Polynomial degree

Use **Polynomial Degree** to choose the regression model used for the standard curve.

Changing the polynomial degree recalculates the curve and updates the derived unknown concentrations. A higher degree may fit the standard points more closely, but the simplest degree that describes the assay response is usually preferred.

Well Data

Review, sort, import, and export per-well assay results.

Use this page to review, sort, import, and export assay well data.

The table combines the assay setup, detected signal values, and calculated concentrations into a per-well data view. Use this page to check the final well results before exporting data or creating a report.

Workflow

Review the well data table, sort rows if needed, then export the data as a CSV file.

You can also import a previously exported well data CSV file to review or reuse saved assay results.

Actions

Help

Shows guidance for this page.



Import Well Data

Loads well data from a CSV file.



Export Well Data

Saves the current well data table as a CSV file.

Table

The table shows one row per well.

The available columns are:

- **Row:** Plate row.
- **Col.:** Plate column.
- **Name:** Well name, such as a standard or unknown sample name.
- **Signal:** Detected signal value from image analysis.
- **Conc.:** Assigned or calculated concentration.
- **Notes:** Notes from the assay setup or imported data.

Click a column header to sort the table by that column. Click again to change the sort direction.

Row ▲	Col.	Name	Signal	Con...	N
A	5		36,70		
A	6		38,42		
A	7		29,99		
A	8		29,13		
A	9	S1	1,94	0,000	
A	10	S9	2,67	0,000	
A	11	U1	31,98	1,840	
A	12	U9	32,34	1,881	
B	1		4,24		
B	2		2,76		
B	3		4,29		
B	4		5,12		
B	5		34,79		
B	6		35,58		
B	7		34,30		
B	8		34,27		
B	9	S2	1,26	0,000	
B	10	S10	2,43	0,000	
B	11	U2	24,24	1,062	
B	12	U10	23,96	1,038	

Review, sort, and import or export the assay well data as CSV.





Figure 8. The Well Data page showing one sortable result row per well.

CSV import and export

Use **Export Well Data** to save the current table as a CSV file.

Use **Import Well Data** to load a saved well data CSV file. The imported file should follow the same structure as an exported well data file.



Windows and macOS

On desktop systems, well data import and export use the workspace folders configured on the **Settings** page.



Android

On Android, **Export Well Data** opens the system file picker with a suggested filename and folder under **Download/Spotxel Reader/Well Data**.



iPhone and iPad

On iOS, **Export Well Data** opens **Save As** with a suggested filename and folder, such as **On My iPhone/Spotxel Reader/Well Data** or **On My iPad/Spotxel Reader/Well Data**.

Spotxel® Reader can read both decimal-point and decimal-comma floating-point numbers. Values are displayed according to your system locale.

Assay Report

Choose report sections and export the assay as a PDF report.

This page combines the current assay data into a single PDF report. The report can include summary information, the assay setup, the plate image, the standard curve, and the well data table.

Workflow

Review the current report data, choose the sections to include, then use **Export Report** to save the report as a PDF file.

After export, the page shows a confirmation message for the exported file.

Actions



Help

Shows guidance for this page.



Export Report

Saves the selected report sections as a PDF file.

Report sections

Choose which sections to include before exporting.

- **Summary:** Includes general assay information, such as assay name, measured color, concentration unit, plate format, well count, number of named standards and unknowns, and the standard curve equation.
- **Assay Setup Snapshot:** Shows the plate layout with named standards, unknowns, and concentration values.
- **Plate Image:** Adds the source plate image used for analysis.
- **Standard Curve:** Adds the standard curve chart and regression information.
- **Well Data Table:** Adds the per-well data table with row, column, name, role, signal, concentration, and notes.

Current data

The **Current Data** area summarizes the data that will be used for the report. Review this area before exporting to confirm that the assay name, measured color, concentration unit, standards, unknowns, and regression equation are correct.

If required data is missing, return to the corresponding page, such as **Image Analysis**, **Assay Setup**, or **Standard Curve**, complete the missing step, and then come back to **Assay Report**.

Report Sections

Choose which report sections to include in the exported PDF.

Sections

☒ Summary
 ☒ Assay Setup Snapshot
 ☒ Plate Image
 ☒ Standard Curve
 ☒ Well Data Table

Current Data

Assay:

Measured Color: Purple

Concentration Unit: ug/mL

Named Standards: 16

Named Unknowns: 16

$Y = 0.0137 - 0.0001X + 0.0018X^2 \quad | \quad R^2 = 0.9926$

Assay report is ready to export.

Choose the report sections, then use Export Report from the action band.

Choose the report sections and export a PDF file.




Figure 9. The Assay Report page with report section selection and a summary of the current assay data.

Exported PDF

The exported PDF is generated from the selected sections. Depending on the selected content and the amount of well data, the report may contain multiple pages.

On desktop systems, exported reports use the workspace folders configured on the **Settings** page.

On Android, **Export Report** opens the system file picker with a suggested filename and folder under **Download/Spotxcel Reader/Reports**.

On iOS, **Export Report** opens **Save As** with a suggested filename and folder, such as **On My iPhone/Spotxcel Reader/Reports** or **On My iPad/Spotxcel Reader/Reports**.

Use the exported PDF for documentation, sharing, archiving, or further review outside Spotxcel® Reader.

BSA

Summary

Generated 3. August 2026 08:55:16 +0200
Measured Color Purple
Concentration Unit ug/mL
Plate Format 96-well
Well Count 96
Regression $Y = 0.0137 - 0.0001X + 0.0018X^2 \mid R^2 = 0.9926$

Assay Setup

Named standards: 16 Named unknowns: 16

	1	2	3	4	5	6	7	8	9	10	11	12
A									S1 0,000	S9 0,000	U1 1,840	U9 1,881
B									S2 0,000	S10 0,000	U2 1,062	U10 1,038
C									S3 0,000	S11 0,000	U3 0,428	U11 0,459
D									S4 0,125	S12 0,125	U4 0,185	U12 0,185
E									S5 0,250	S13 0,250	U5 0,079	U13 0,076
F									S6 0,500	S14 0,500	U6 0,027	U14 0,026
G									S7 1,000	S15 1,000	U7 0,028	U15 0,026
H									S8 2,000	S16 2,000	U8 0,030	U16 0,024

Page 1 of 8

Plate Image

Source image: sample3.jpg

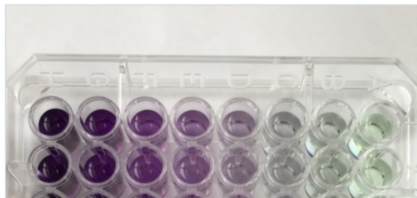


Figure 10. The exported Assay Report displayed in a PDF viewer, showing the first page and the beginning of the second page.

Purchases

Review licenses, subscriptions, entitlements, and purchase restoration.

Spotxel® Reader is a free app. The unpaid version is feature-complete and includes a small advertising placement. Paid access removes this advertising placement.

Paid access is available through purchase products provided by your platform store.

Paid access options

- **Perpetual License:** Permanently removes advertising.
- **3-Month Subscription:** Removes advertising while the subscription is active. It renews every three months, and a free trial may be available depending on the store and current offer.

On Apple platforms, a perpetual license purchased on iPhone, iPad, or Mac can be restored on another Apple device when the same Apple App Store account is used.

Prices, currencies, taxes, trial availability, renewal rules, cancellation, and refunds are handled by the platform store.

Workflow

Select a purchase product, then choose **Buy now** or **Start plan**.

The platform store, such as Microsoft Store, Apple App Store, or Google Play, handles the purchase process. Spotxel® Reader receives the purchase result after you complete or cancel the transaction.

Active paid access is shown in the **Entitlements** section.

Actions

Help

Shows guidance for this page.

Refresh

Reloads the product catalog and entitlement state from the store backend.

Restore

Restores previous purchases for the currently signed-in store account, if supported by the platform store.

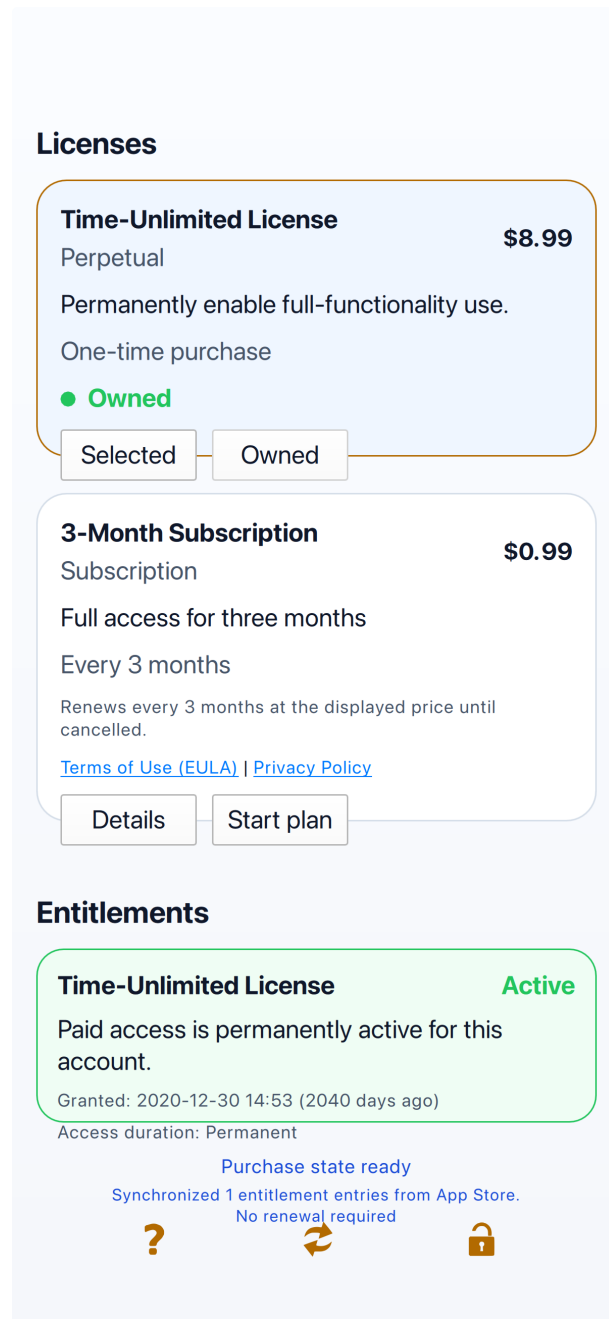


Figure 11. The iOS Purchases page, showing App Store products and current entitlement status.

Licenses

The **Licenses** section lists the available purchase products.

Select a product to view or purchase it. Depending on the product and store state, available buttons may include **Details**, **Buy now**, **Start plan**, **Selected**, or **Current plan**.

Entitlements

The **Entitlements** section shows whether paid access is active.

If a license or subscription is active, this section shows the active entitlement and, where available, the access period. If no paid entitlement is active, Spotxel® Reader runs in ad-supported mode.

Problems with purchases

If paid access is not shown after a purchase, first check the following:

- The device is connected to the internet.
- You are signed in with the same store account used for the purchase.
- On Windows, check the Microsoft Store account.
- On macOS or iOS, check the Apple App Store account.
- On Android, check the Google Play account.

Then use **Refresh** to reload the product catalog and entitlement state. Check the status message at the bottom of the page to confirm whether the store connection succeeds.

If the entitlement is still missing, use **Restore** to restore previous purchases for the current store account.

If the problem remains, [contact SICASYS support](#) and include a short description of the issue, your platform, and the purchase product involved. We will help verify the purchase state and guide you through the next steps.

Settings

Configure appearance, workspace, camera, grid defaults, and diagnostics.

Settings apply immediately where possible and are used by related pages such as **Camera** and **Image Analysis**.

Actions

Help

Shows guidance for this page.

Menu

Opens the navigation menu.

Settings groups

- **Appearance:** Configures the color profile and appearance mode.
- **Rotate:** Changes the desktop layout orientation where available.
- **Workspace:** Shows where Spotxel® Reader stores working files and where exported files are saved.
- **Camera Device:** Selects the camera used for image capture.
- **Grid:** Configures the default microplate grid type, visibility, size, and distortion.
- **Troubleshooting:** Enables support-level diagnostic logging and shows the active log path.

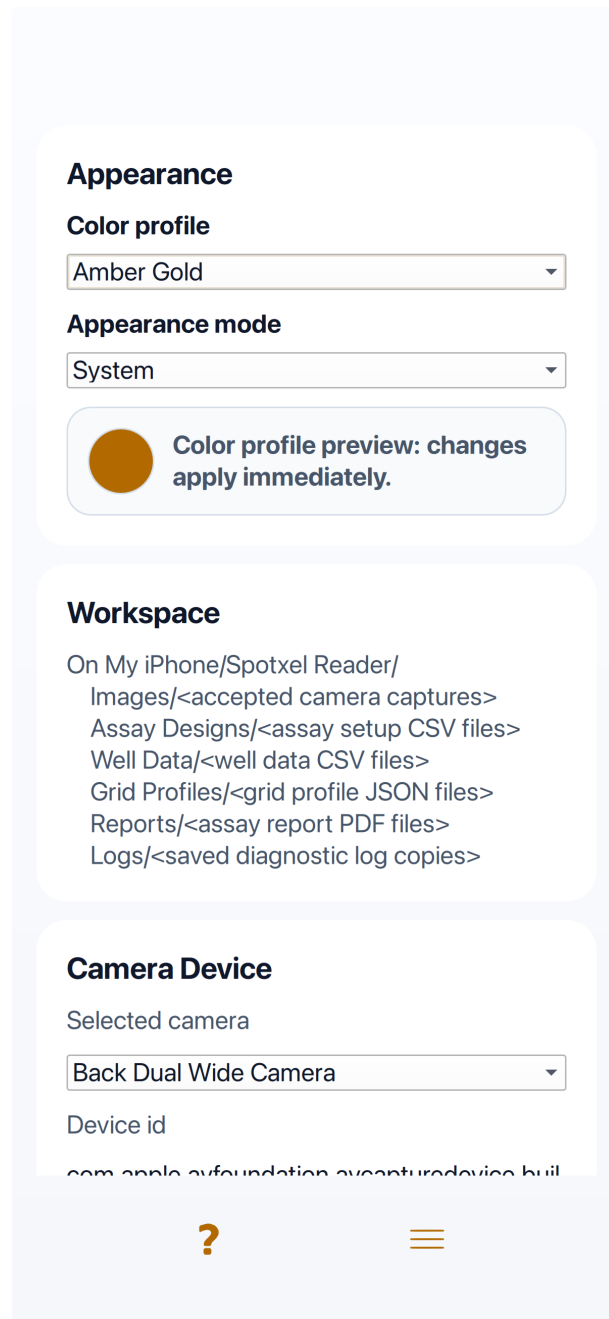


Figure 12. The iOS Settings page, showing appearance options, workspace locations, and camera selection.

Appearance

Use **Appearance** to adjust the visual style of Spotxcel® Reader.

Color profile

The **Color profile** setting changes the accent color used for buttons, highlights, and selected controls. The preview shows the selected color profile, and changes apply immediately.

Appearance mode

The **Appearance mode** setting controls whether the app uses a light or dark visual style.

- **System:** Follows the system appearance.

- **Light:** Uses the light appearance.
- **Dark:** Uses the dark appearance.

Rotate



Windows and macOS

Use **Rotate** to switch the desktop layout orientation where this is supported.

Portrait mode can be useful on narrow screens or tablet-style displays. Landscape mode is recommended for most desktop workflows because it provides more horizontal space for assay pages, tables, and charts.

Workspace

Use **Workspace** to review where files created or used by Spotxel® Reader are stored.

Accepted camera captures can be opened again from the **Image Analysis** page by using **Open Image**.



Windows and macOS

On desktop systems, the workspace can be changed. By default, the workspace is created in the user's Documents folder as **Spotxel Reader**. Save and export dialogs use workspace subfolders as their starting locations, making related files easier to find and reuse.

Use **Change** to select another workspace folder. Use **Reset to Default** to return to the default workspace location. Use **Open Folder** to open the current workspace in the system file manager. These controls are hidden on Android and iOS because those platforms use system-managed locations.



Android

On Android, accepted camera captures are automatically stored under:

- **Pictures/Spotxel Reader**

For files generated by the app, the following default save locations are suggested:

- **Download/Spotxel Reader/Assay Designs:** Assay setup and assay design CSV files.
- **Download/Spotxel Reader/Well Data:** Well data CSV files.
- **Download/Spotxel Reader/Grid Profiles:** Grid profile JSON files.
- **Download/Spotxel Reader/Reports:** Assay report PDF files.
- **Download/Spotxel Reader/Logs:** Diagnostic log copies saved from Troubleshooting.

For generated documents, the Android system file picker may allow you to change the file name and save location.



iPhone and iPad

On iOS, the following default save locations are suggested. In the Files app, the device location may appear as **On My iPhone**, **On My iPad**, or a localized equivalent, depending on the device and system language. The paths below use **On My Device** as a generic label.

- **On My Device/Spotxel Reader/Images:** Accepted camera captures.
- **On My Device/Spotxel Reader/Assay Designs:** Assay setup and assay design CSV files.
- **On My Device/Spotxel Reader/Well Data:** Well data CSV files.
- **On My Device/Spotxel Reader/Grid Profiles:** Grid profile JSON files.
- **On My Device/Spotxel Reader/Reports:** Assay report PDF files.
- **On My Device/Spotxel Reader/Logs:** Diagnostic log copies saved from Troubleshooting.

For generated documents, **Save As** may allow you to change the file name and save location.

Camera Device

Use **Camera Device** to select the camera used by the **Camera** page.

The **Selected camera** list shows the available camera devices. After selecting a camera, the device identifier and permission state are shown below.

If the expected camera is not available, check that it is connected, not being used by another application, and permitted by the operating system.

Grid

Use **Grid** to configure the default microplate grid behavior.

The **Grid type** setting selects the microplate grid format used for analysis. The standard microplate grid is **Microplate (12 × 8)**.

The **Grid visible** setting controls whether the grid is shown by default.

The grid controls also show the current grid mode, grid shape, cell width, and distortion. Use these settings as a starting point for camera capture and image analysis. The grid can still be adjusted later on the **Camera** and **Image Analysis** pages.

Troubleshooting

Use **Troubleshooting** to enable detailed diagnostic logging when support asks for a trace.

Detailed logging records additional runtime information, such as image loading, camera capture, grid alignment, analysis steps, workspace access, and purchase-backend status. It is disabled by default and should normally remain disabled.

When detailed logging is enabled, the current private log path is shown in a shortened, user-friendly form.

On Android and iOS, use **Save Log Copy** to save the current log entries as a stable copy in a user-accessible location. The saved copy can then be reviewed or shared with support.



Android

On Android, saved log copies are stored under:

- **Download/Spotxel Reader/Logs**



iPhone and iPad

On iOS, saved log copies are stored under:

- **On My Device/Spotxel Reader/Logs**

Saving a copy does not move, replace, or interrupt the active private log. Repeating the action creates another saved copy without overwriting an existing one.

The log file may contain technical details such as file paths, device information, and store/backend status messages. **Review** the file before sharing it if it may contain sensitive information.

Third-Party Software Notices

Notices and license terms for common and platform-specific third-party components.

Spotxel Reader includes or uses the following third-party runtime software components and relevant model attributions.

OpenCV

Copyright (c) OpenCV team.

OpenCV is licensed under the Apache License, Version 2.0.

AI model

Spotxel Reader includes an AI model developed by SICASYS.

The model was developed and trained using TensorFlow/Keras, including Keras MobileNetV3Small weights pretrained on ImageNet. It was converted for use with the platform-specific inference engine.

TensorFlow and Keras are licensed under the Apache License, Version 2.0.

Apache License, Version 2.0

Version 2.0, January 2004

<http://www.apache.org/licenses/>

TERMS AND CONDITIONS FOR USE, REPRODUCTION, AND DISTRIBUTION

1. Definitions.

"License" shall mean the terms and conditions for use, reproduction, and distribution as defined by Sections 1 through 9 of this document.

"Licensor" shall mean the copyright owner or entity authorized by the copyright owner that is granting the License.

"Legal Entity" shall mean the union of the acting entity and all other entities that control, are controlled by, or are under common control with that entity. For the purposes of this definition, "control" means (i) the power, direct or indirect, to cause the direction or management of such entity, whether by contract or otherwise, or (ii) ownership of fifty percent (50%) or more of the outstanding shares, or (iii) beneficial ownership of such entity.

"You" (or "Your") shall mean an individual or Legal Entity exercising permissions granted by this License.

"Source" form shall mean the preferred form for making modifications, including but not limited to software source code, documentation source, and configuration files.

"Object" form shall mean any form resulting from mechanical transformation or translation of a Source form, including but not limited to compiled object code, generated documentation, and conversions to other media types.

"Work" shall mean the work of authorship, whether in Source or Object form, made available under the License, as indicated by a copyright notice that is included in or attached to the work.

"Derivative Works" shall mean any work, whether in Source or Object form, that is based on, or derived from, the Work and for which the editorial revisions, annotations, elaborations, or other modifications represent, as a whole, an original work of authorship. For the purposes of this License, Derivative Works shall not include works that remain separable from, or merely link or bind by name to the interfaces of, the Work and Derivative Works thereof.

"Contribution" shall mean any work of authorship, including the original version of the Work and any modifications or additions to that Work or Derivative Works thereof, that is intentionally submitted to Licensor for inclusion in the Work by the copyright owner or by an individual or Legal Entity authorized to submit on behalf of the copyright owner. For the purposes of this definition, "submitted" means any form of electronic, verbal, or written communication sent to the Licensor or its representatives, including but not limited to communication on electronic mailing lists, source-code control systems, and issue-tracking systems that are managed by, or on behalf of, the Licensor for the purpose of discussing and improving the Work, but excluding communication that is conspicuously marked or otherwise designated in writing by the copyright owner as "Not a Contribution."

"Contributor" shall mean Licensor and any individual or Legal Entity on behalf of whom a Contribution has been received by Licensor and subsequently incorporated within the Work.

2. Grant of Copyright License.

Subject to the terms and conditions of this License, each Contributor hereby grants to You a perpetual, worldwide, non-exclusive, no-charge, royalty-free, irrevocable copyright license to reproduce, prepare Derivative Works of, publicly display, publicly perform, sublicense, and distribute the Work and such Derivative Works in Source or Object form.

3. Grant of Patent License.

Subject to the terms and conditions of this License, each Contributor hereby grants to You a perpetual, worldwide, non-exclusive, no-charge, royalty-free, irrevocable patent license to make, have made, use, offer to sell, sell, import, and otherwise transfer the Work, where such license applies only to those patent claims licensable by such Contributor that are necessarily infringed by their Contribution alone or by combination of their Contribution with the Work to which such Contribution was submitted. If You institute patent litigation against any entity alleging that the Work or a Contribution incorporated within the Work constitutes direct or contributory patent infringement, then any patent licenses granted to You under this License for that Work shall terminate as of the date such litigation is filed.

4. Redistribution.

You may reproduce and distribute copies of the Work or Derivative Works thereof in any medium, with or without modifications, and in Source or Object form, provided that You meet the following conditions:

- (a) You must give any other recipients of the Work or Derivative Works a copy of this License; and
- (b) You must cause any modified files to carry prominent notices stating that You changed the files; and

(c) You must retain, in the Source form of any Derivative Works that You distribute, all copyright, patent, trademark, and attribution notices from the Source form of the Work, excluding those notices that do not pertain to any part of the Derivative Works; and

(d) If the Work includes a "NOTICE" text file as part of its distribution, then any Derivative Works that You distribute must include a readable copy of the attribution notices contained within such NOTICE file, excluding those notices that do not pertain to any part of the Derivative Works, in at least one of the following places: within a NOTICE text file distributed as part of the Derivative Works; within the Source form or documentation, if provided along with the Derivative Works; or within a display generated by the Derivative Works, if and wherever such third-party notices normally appear. The contents of the NOTICE file are for informational purposes only and do not modify the License. You may add Your own attribution notices within Derivative Works that You distribute, alongside or as an addendum to the NOTICE text from the Work, provided that such additional attribution notices cannot be construed as modifying the License.

You may add Your own copyright statement to Your modifications and may provide additional or different license terms and conditions for use, reproduction, or distribution of Your modifications, or for any such Derivative Works as a whole, provided Your use, reproduction, and distribution of the Work otherwise complies with the conditions stated in this License.

5. Submission of Contributions.

Unless You explicitly state otherwise, any Contribution intentionally submitted for inclusion in the Work by You to the Licensor shall be under the terms and conditions of this License, without any additional terms or conditions. Notwithstanding the above, nothing herein shall supersede or modify the terms of any separate license agreement You may have executed with Licensor regarding such Contributions.

6. Trademarks.

This License does not grant permission to use the trade names, trademarks, service marks, or product names of the Licensor, except as required for reasonable and customary use in describing the origin of the Work and reproducing the content of the NOTICE file.

7. Disclaimer of Warranty.

Unless required by applicable law or agreed to in writing, Licensor provides the Work, and each Contributor provides its Contributions on an "AS IS" BASIS, WITHOUT WARRANTIES OR CONDITIONS OF ANY KIND, either express or implied, including, without limitation, any warranties or conditions of TITLE, NON-INFRINGEMENT, MERCHANTABILITY, or FITNESS FOR A PARTICULAR PURPOSE. You are solely responsible for determining the appropriateness of using or redistributing the Work and assume any risks associated with Your exercise of permissions under this License.

8. Limitation of Liability.

In no event and under no legal theory, whether in tort, contract, or otherwise, unless required by applicable law or agreed to in writing, shall any Contributor be liable to You for damages, including any direct, indirect, special, incidental, or consequential damages of any character arising as a result of this License or out of the use or inability to use the Work, including but not limited to damages for loss of goodwill, work stoppage, computer failure or malfunction, or any and all other commercial damages or losses, even if such Contributor has been advised of the possibility of such damages.

9. Accepting Warranty or Additional Liability.

While redistributing the Work or Derivative Works thereof, You may choose to offer, and charge a fee for, acceptance of support, warranty, indemnity, or other liability obligations or rights consistent with this License. However, in accepting such obligations, You may act only on Your own behalf and on Your sole responsibility, not

on behalf of any other Contributor, and only if You agree to indemnify, defend, and hold each Contributor harmless for any liability incurred by, or claims asserted against, such Contributor by reason of Your accepting any such warranty or additional liability.

END OF TERMS AND CONDITIONS

Android-specific components

TensorFlow Lite

Spotxel Reader for Android includes the TensorFlow Lite runtime for on-device AI inference.

TensorFlow Lite is licensed under the Apache License, Version 2.0.

macOS and iOS-specific components

No additional third-party inference runtime is bundled for Apple builds. Spotxel Reader uses Apple's system Core ML framework provided by macOS and iOS.

Windows-specific components

ONNX

Copyright (c) ONNX Project Contributors.

ONNX is licensed under the Apache License, Version 2.0.

ONNX Runtime

Copyright (c) Microsoft Corporation.

ONNX Runtime is licensed under the MIT License.

Additional third-party notices for ONNX Runtime are provided in the ONNX Runtime ThirdPartyNotices file distributed with this application.

MIT License

Copyright (c) Microsoft Corporation

Permission is hereby granted, free of charge, to any person obtaining a copy of this software and associated documentation files (the "Software"), to deal in the Software without restriction, including without limitation the rights to use, copy, modify, merge, publish, distribute, sublicense, and/or sell copies of the Software, and to permit persons to whom the Software is furnished to do so, subject to the following conditions:

The above copyright notice and this permission notice shall be included in all copies or substantial portions of the Software.

THE SOFTWARE IS PROVIDED "AS IS", WITHOUT WARRANTY OF ANY KIND, EXPRESS OR IMPLIED, INCLUDING BUT NOT LIMITED TO THE WARRANTIES OF MERCHANTABILITY, FITNESS FOR A PARTICULAR PURPOSE AND NONINFRINGEMENT. IN NO EVENT SHALL THE AUTHORS OR COPYRIGHT HOLDERS BE LIABLE FOR ANY CLAIM,

DAMAGES OR OTHER LIABILITY, WHETHER IN AN ACTION OF CONTRACT, TORT OR OTHERWISE, ARISING FROM, OUT OF OR IN CONNECTION WITH THE SOFTWARE OR THE USE OR OTHER DEALINGS IN THE SOFTWARE.